

TEST DEVICE FOR HIP JOINT CUPS ABRASION TESTS AND EXPERIMENTAL EVALUATION OF ABRASION

Martin Houfek, Vladimir Fuis and Lubomir Houfek

Institute of Solid Mechanics, Mechatronics and Biomechanics, Faculty of Mechanical Engineering, Brno University of Technology, Czech Republic, houfek.m@fme.vutbr.cz

INTRODUCTION

Problems of artificial joints are actual problems in orthopedics today, occurring in both older and productive age people. The problems of joint cup abrasion are actual for patients after the surgery due to hip joint attrition or injury and for oncology patients. Therefore nowadays the medical system is interested in reliability of bioimplants, that is based apart from stress/strain analysis also on determination of abrasion properties and loss of material caused by common life style of a patient. The hip joint abrasion tests are currently actual and therefore we designed and implemented experimental device for experimental testing of hip joint prosthesis abrasion.

METHODS

Test device is equipped with two MAXON RE36 DC drives and planetary gearboxes MAXON GB42. Upper tray is connected with actuator through flexible joint. Upper actuator simulates one part of combined motion (walking), that is inclination. The main step is simulated by lower actuator (step forward). Lower actuator is connected with clevis containing the head of hip joint. The tray with cast-in joint cup is connected through flexible joint with upper element. Actuators of the test device are controlled by EPOS unit by MAXON (Figure 1).



Figure 1: Experimental device

The test element is mounted rigidly with high precision due to consecutive evaluation of abrasion using optics method. For mounting we used cup cast-in to DENTACRYL. This mounting method seems to be the most suitable for our

requirements (Figure 2). The test element mounted this way is put into the test device and tested.

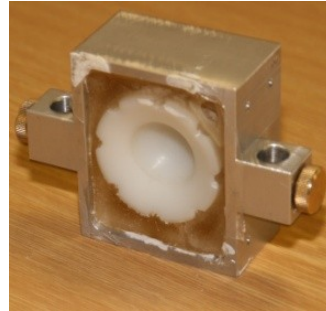


Figure 2: Cast-in hip joint cup

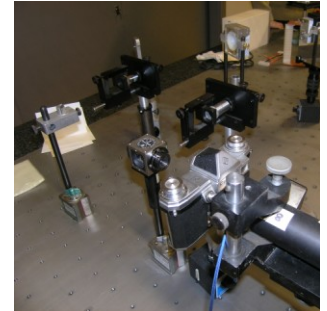


Figure 3: Interferometric method

To evaluate the abrasion we used single hologram optical method [1]. This method is based on the interference of reconstructed hologram wave with the wave coming from the object. So first a hologram is made for the test element. This hologram is put into its original location and test element is lit through the hologram. The light coming through the hologram is unchanged, but whenever there are changes in the test element the light is reflected in different direction and interference fringes occur (Figure 3) [2].

The creation and position of the fringes quantitatively is obtained by reconstructed wave description according to:

$$u_1 = \bar{u}_1 + \chi u_c u_R^* u_s + \chi u_c u_R u_s^*$$

RESULTS AND DISCUSSION

After performing the test on the sample of hip joint cup with no wear we verified that we are able to perform real measurement of abrasion using single hologram method. During the initial test stage we verified the method on hip joint cup with no wear where no interference occurred, which matches reality.

CONCLUSIONS

The experiment can be concluded with the statement that the method of mounting the cup in the bed and in optical channel enables the measurement of material wear with holographic method.

ACKNOWLEDGEMENTS

Published results were acquired using the subsidisation of the Ministry of Education, Youth and Sports of the Czech Republic, research plan MSM0021630518.

This research was supported by the Ministry of Education, Youth and Sports of the Czech Republic (project 2E08017).

REFERENCES

1. Janicek P., Experimental modeling, Brno, 1999.
2. Brooks, R. et al. Holographic Photography of High-Speed Phenomena with Conventional and Q-Switched Ruby Lasers. Appl. Phys. Lett., 7, 1965, p. 92.